

NONPOROUS ELECTRODE

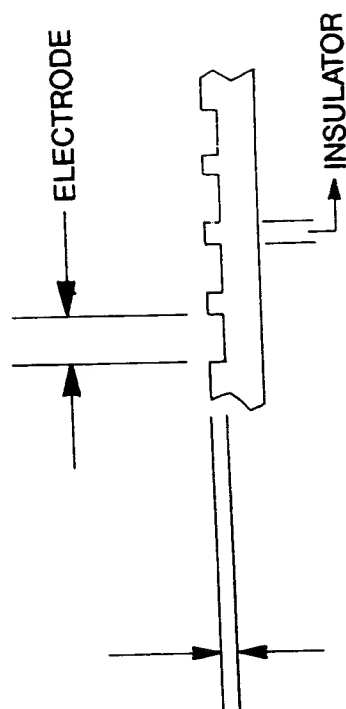
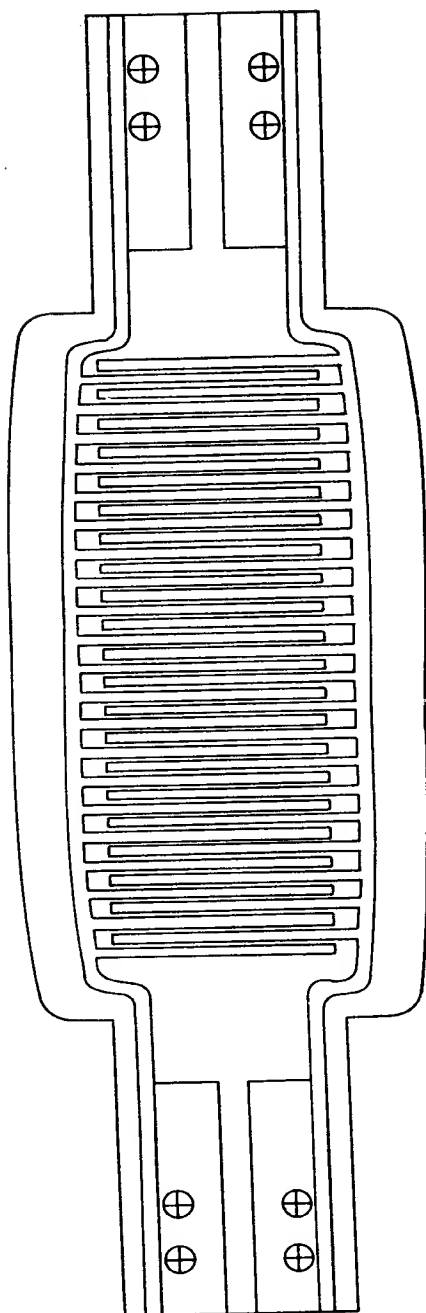


FIG. 7

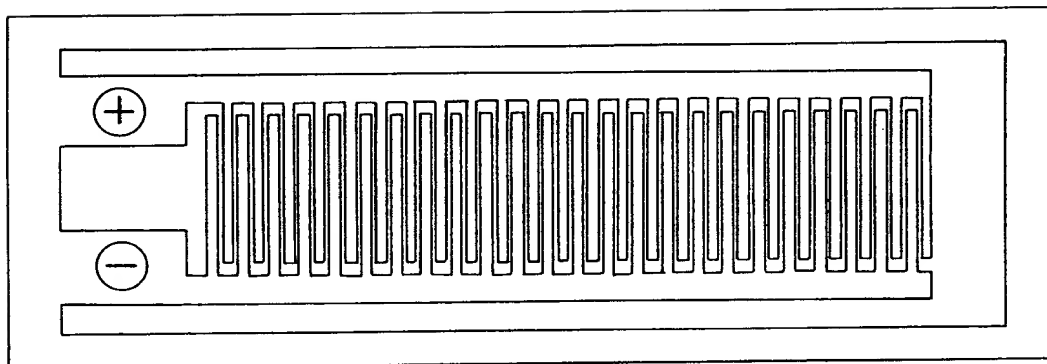


FIG. 1

INFORMATION CONTAINED  
HEREIN IS UNCLASSIFIED  
DATE 10-10-2001 BY 60322  
1007/100

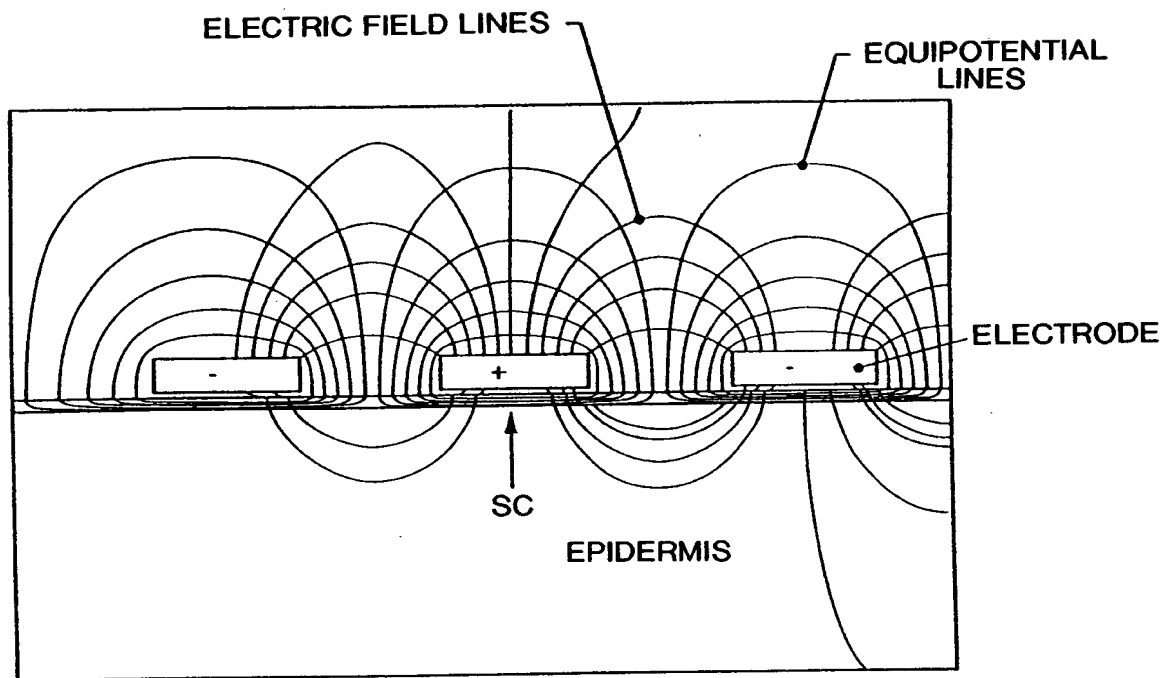


FIG. 2

FIELD STRENGTH BELOW AN ELECTRODE  
BEFORE BREAKDOWN OF THE S.C.

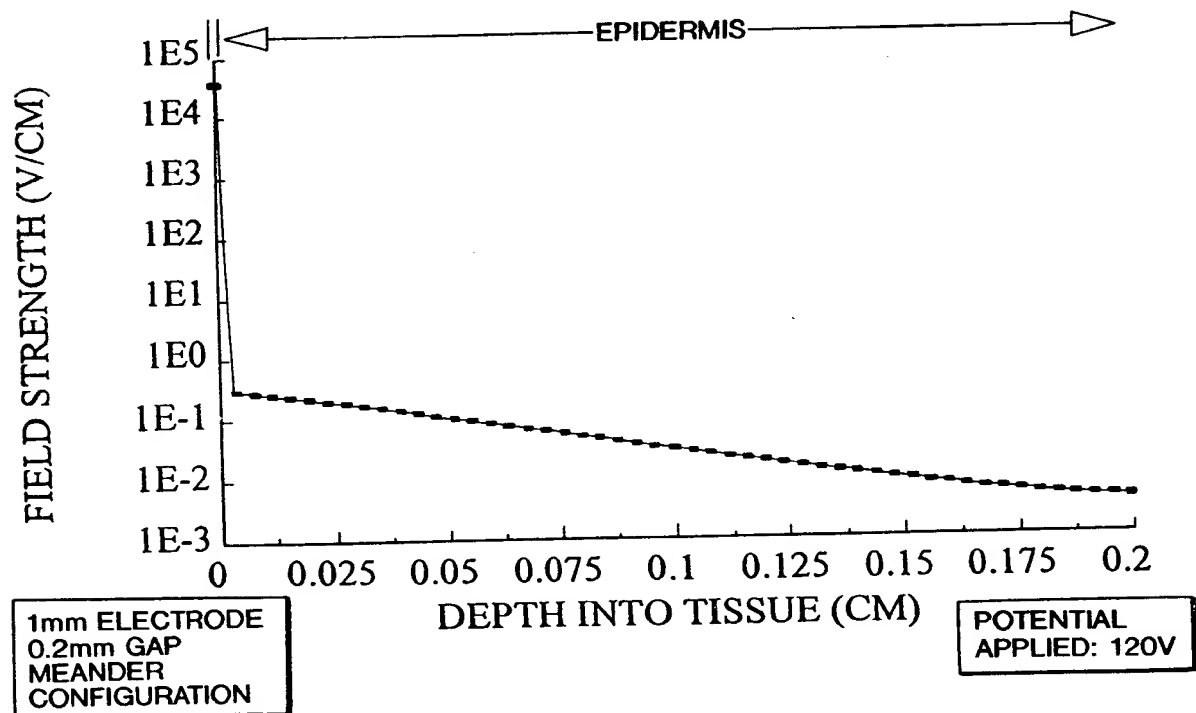


FIG. 3A

FIELD STRENGTH BELOW AN ELECTRODE  
AFTER BREAKDOWN OF THE S.C.

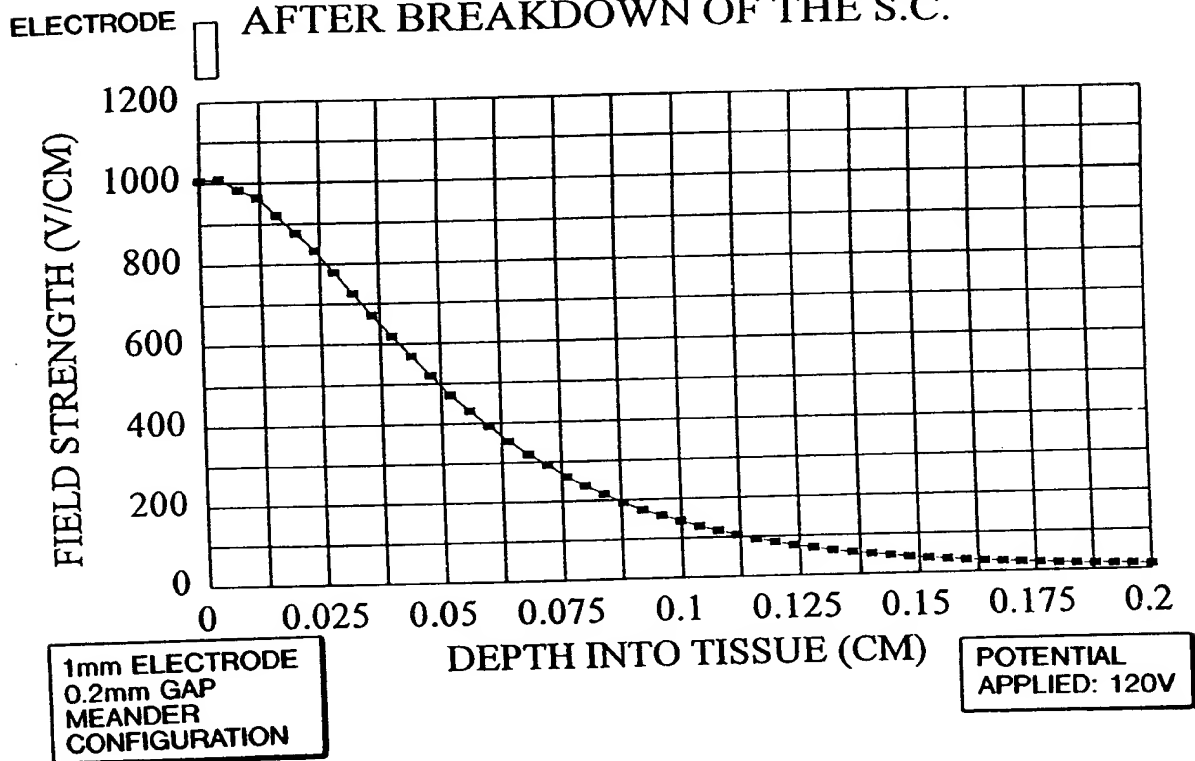


FIG. 3B

50H 12  
TAP 12  
120V 120V  
120V 120V  
120V 120V

## Field Across Tissue

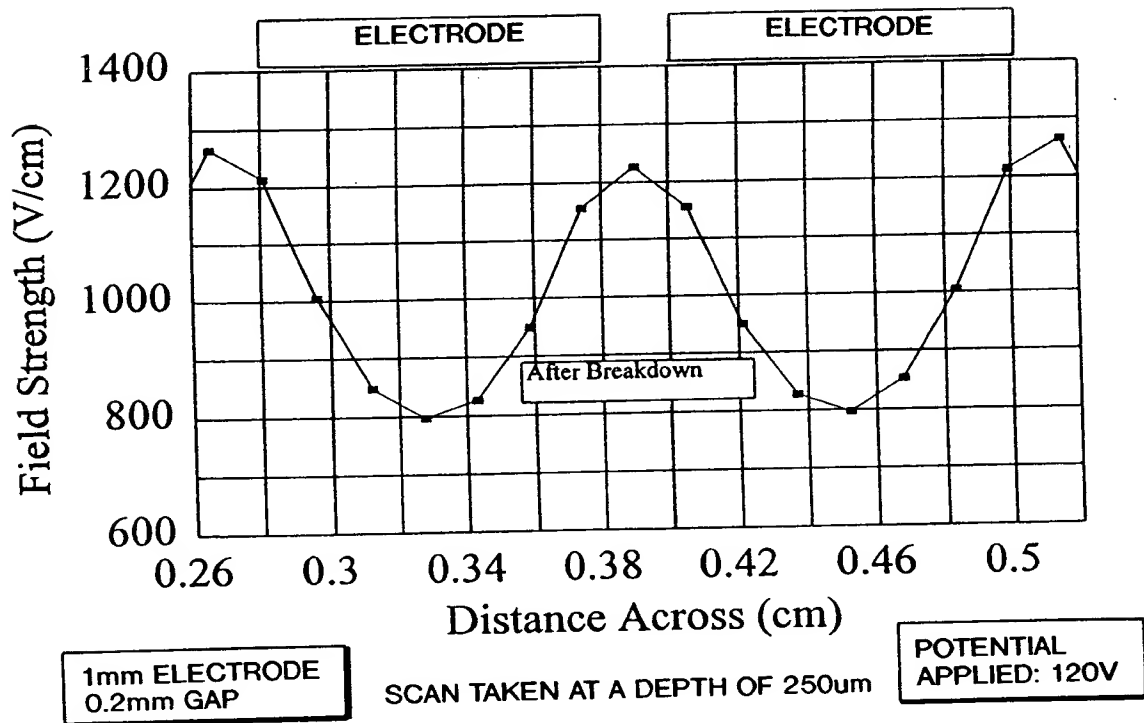


FIG. 4A

## Field Across Tissue

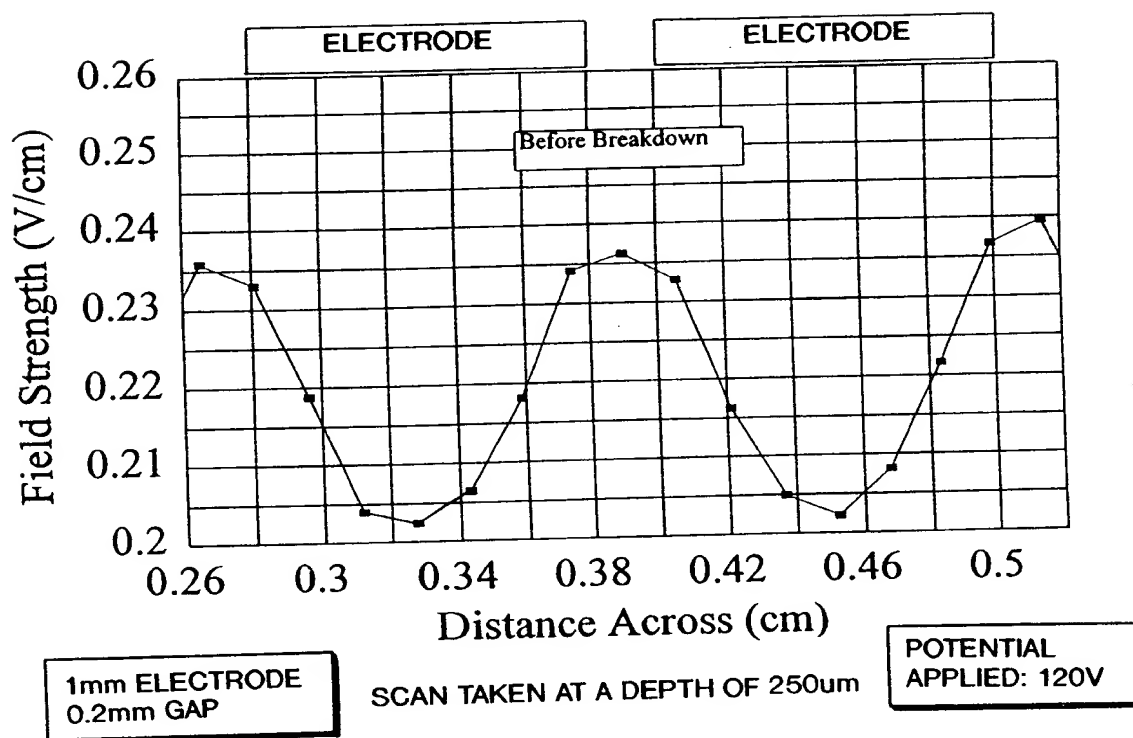


FIG. 4B

BATTERY-POWERED  
HAND HELD PULSER

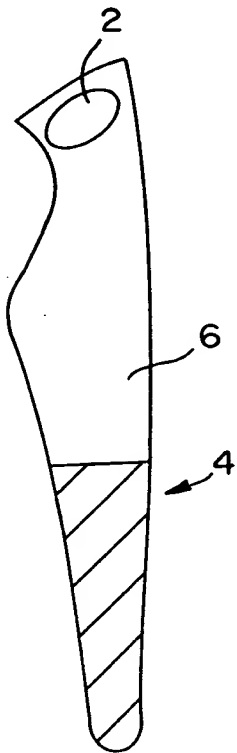


FIG. 5A

BATTERY-POWERED  
HAND HELD PULSER

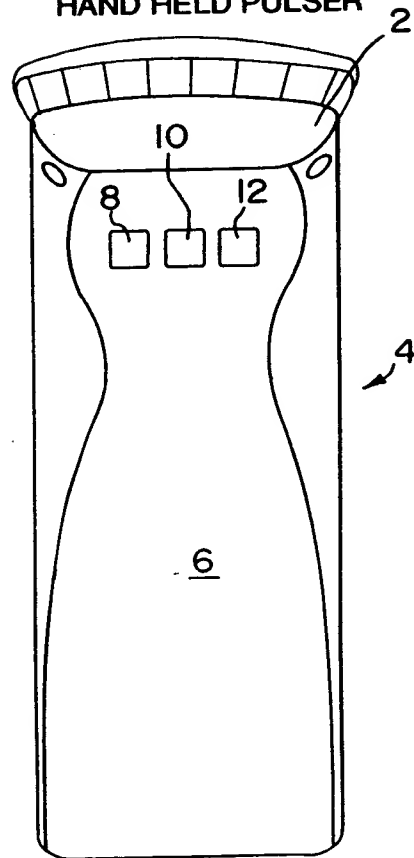


FIG. 5B

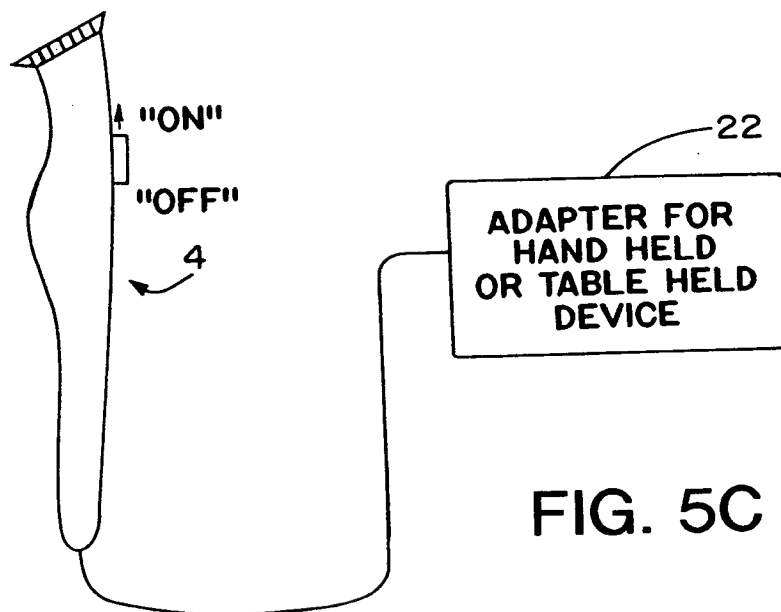


FIG. 5C





FIG. 6A

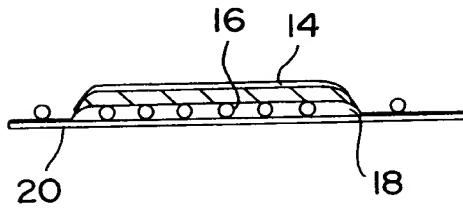


FIG. 6B



FIG. 6C




FIG. 6D




FIG. 6E